# The Phi Fan Performance Standard (PFPS)

**Revision 2.1**

**Author: Aristeidis Bitziopoulos**

**Nicosia, Cyprus**
October 2026

## Revision History

| Version | Release Date | Notes |
|---|---|---|
| 1.0 | May 2024 | First draft |
| 1.1 | June 2024 | Change in the badges. Fan diameter was omitted. |
| 1.2 | August 2026 | Measurement uncertainties updated to the current controlled budgets (P19). |
| 1.3 | August 2026 | Measurement uncertainties corrected: Type B contributions already contained within the Type A term were removed as double counted (P19 rev.05, 07-08-2026). |
| 1.4 | August 2026 | Decision rule for the award of PFPS badges stated: simple acceptance, with a repeat-and-mean rule at level boundaries. |
| 1.5 | August 2026 | Chamber noise floor stated as around 6 dB(A) rather than < 6 dB(A), for consistency with the other Cybenetics test documents. |
| 1.6 | September 2026 | Measurement uncertainties re-derived on a new control-sample base: the twelve control runs of 02/03-09-2026 replace the previous fifteen-run base (P19-F01 rev.07, 07-09-2026). Static pressure U 2.422 to 0.6727 Pa; air flow relative component 1.9296 % to 1.23176 %, U 5.000 to 4.290 CFM at the control point. |
| 1.7 | September 2026 | Translation alignment only, no change to any measured value or declared uncertainty. The German, Traditional Chinese and Simplified Chinese editions carried a shortened form of the air-flow uncertainty sentence, with untranslated English inside it; all three now carry the same three-sentence wording as this English edition. |
| 1.8 | September 2026 | Document presentation corrected: the cover date is September 2026, the translated dates for revisions 1.6 and 1.7 match the English history, duplicate or untranslated contents headings are removed, and compact rating and uncertainty tables are kept together across page breaks. No measured value, test, declared uncertainty or published rating changes. The contents starts on its own page and excludes body text accidentally marked as a heading. |
| 1.9 | October 2026 | Fans whose maximum noise output is below 25 dBA are now rated at their measured 20 dBA normalized noise output, against new 20 dBA requirements derived from the 25 dBA requirements with the median 25 dBA to 20 dBA ratios of 194 fans measured at both levels. Previously these fans could not be rated. The 25 dBA requirements, the test procedure and the declared measurement uncertainties are unchanged, and no existing rating changes. |
| 2.0 | October 2026 | References re-checked on 03-10-2026: dead and moved links replaced with the manufacturers' and publishers' current pages, access dates updated. |
| 2.1 | October 2026 | Platinum, Titanium and Diamond requirements raised for airflow and static pressure, in both fan categories and at both 25 dBA and 20 dBA; fans larger than 140mm are rated with the 135/140mm requirements; all existing ratings re-assessed from their measurements. |

# Table of Contents

Prologue ..... 4
Fan Operation & Bearing Types ..... 4
Test Equipment ..... 5
Fan Performance: P-Q Curve ..... 7
Normalized Noise Testing ..... 8
Noise Measurements Procedure ..... 9
The Phi Fan Performance Standard - PFPS ..... 10
Performance Badges & Ratings ..... 12
Measurement Uncertainty ..... 13
Decision Rule ..... 14
Epilogue ..... 14
References ..... 15

## Prologue

Fans are everywhere, cooling down sensitive to heat electronic devices. They are often overlooked unless noisy because they just do their job for long periods until they stop spinning. This article aims to explain in detail how we evaluate cooling fans and how we rate them according to their performance.

## Fan Operation & Bearing Types

The most crucial components of every fan are its bearing and shaft, to which the fan blade is attached. The bearing is a stationary cylinder inside which the shaft rotates. To provide high reliability and decreased noise output, friction between the shaft and the bearing has to be minimized. In most cases, oil is used as a lubricant. However, other methods can be used as well (for instance, Teflon-coated surfaces). If the oil isn't sealed properly inside the bearing, its quantity will diminish as time passes, increasing friction, leading to slower fan rotation and increased noise, until the fan breaks down and stops rotating.

The most popular bearing types used in PC cooling fans are the following:

- Sleeve bearing
- Rifle bearing
- Double ball (DBB) bearing
- Fluid dynamic bearing (FDB) and hydro dynamic bearing (HDB)
- Magnetic bearing

It is beyond this article's purpose to explain in detail the various bearing types, but briefly, sleeve bearing fans are the less reliable ones. Rifle-bearing fans offer enhanced reliability, while FDB and HDB fans are even more reliable.

Double ball bearing fans are highly tolerant to increased temperatures but typically have bearing noises at low speeds, while magnetic bearing fans have the same tolerance at high temperatures as DBB fans, without any bearing noises at low speeds.

Other bearing types exist, but they are usually improved versions of the bearing listed above, under a different name.

## Test Equipment

The main instrument we use for fan measurements is an LW-9266 Fan PQ performance measurement apparatus [1]. This is a highly sophisticated scientific instrument made in Taiwan by Long Win.

LW-9266 Technical Specifications

- Manufacturer: Long Win Science & Technology Corporation
- Air Flow Rate: 2.4 – 250 CFM
- Accuracy of Air Flow Rage: <3.5% INFS
- Repeatability error: < 2%
- Static pressure: 0-20mmAq (100mmAq with the high static pressure throttle device)
- Overall Dimensions: 0.7 (W) x 2.2 (L) x 1.6 (H) m
- Power Source: 220VAC, 5A, Single Phase, 50/60Hz
- Based on Standards: ISO 5801-2007, AMCA 210-0, ASHRAE 51-2007, IEC 61591-2005, GB/T 1236-200

Besides the Long Win machine, we also use the following equipment.

- Noise Test Environment: Hemi-Anechoic Chamber with a noise floor of around 6 dB(A)
- Conditions: 25 (+-2) degrees Celsius, 40-50% humidity
- Sound Analyzer: Bruel & Kjaer 2270-S G4
- Microphone: Bruel & Kjaer Type 4955-A

- Mic Calibrator:  Bruel & Kjaer Type 4231
- Data Logger: Picoscope TC-08 [2]

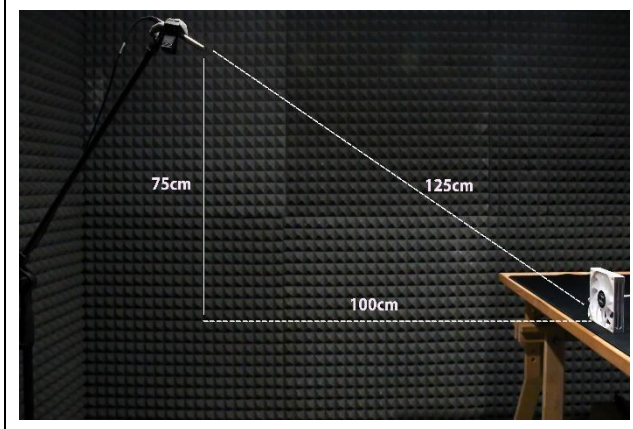


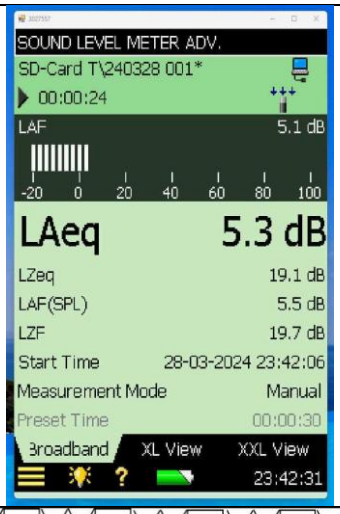


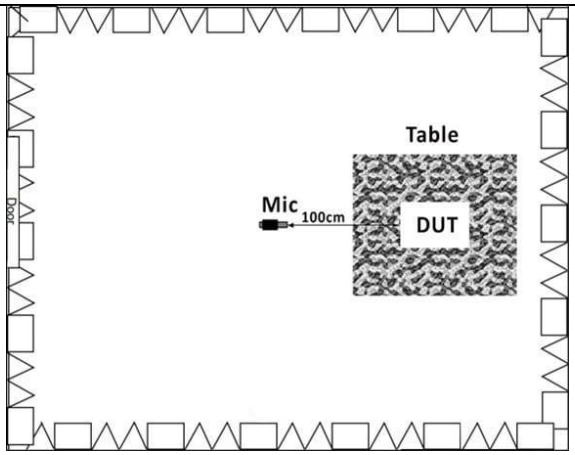


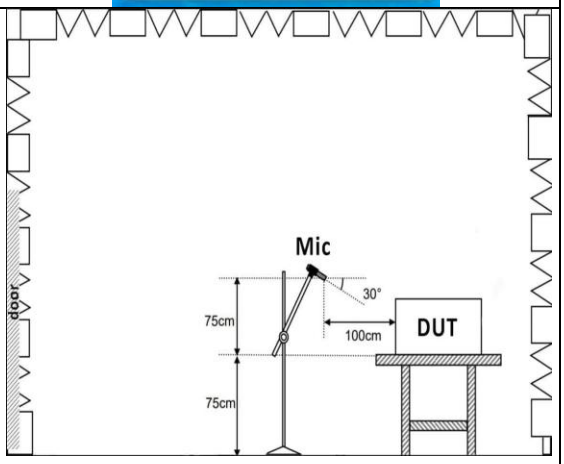


The measuring microphone is positioned in such a way that it forms a 30$^{o}$ to 45$^{o}$ degree angle to the horizontal axis, and its vertical distance from the Device Under Test (DUT) is one meter.

## Fan Performance: P-Q Curve

Regardless of its dimensions, every fan, whether DC or AC-powered, has a characteristic curve called P-Q. This curve shows the correlation between the fan's airflow and its static pressure. With the letter "P," we describe static pressure, and with "Q," airflow.

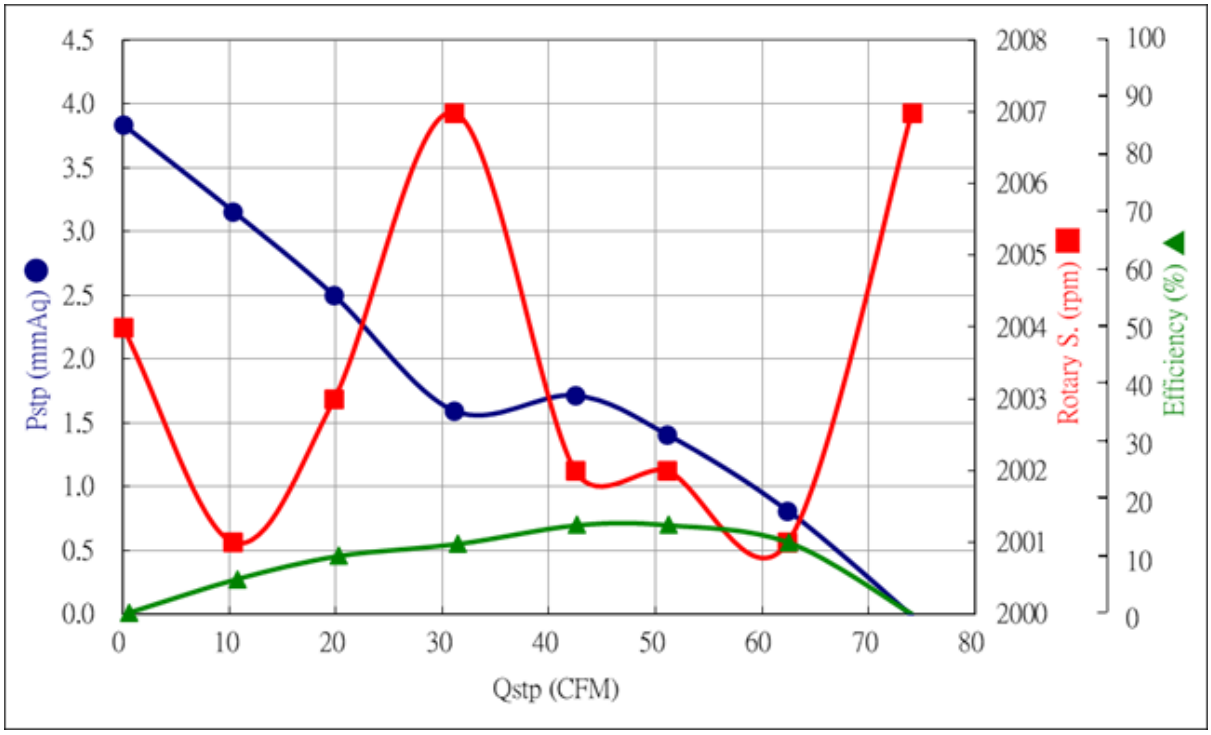


When we refer to a fan's airflow, we speak about the total amount of air the fan pushes or produces per unit of time. Airflow is usually measured in Cubic Feet per Minute (CFM). Fan manufacturers measure a fan's CFM in an open environment without any obstacles in front of it, and this plays a huge role, as you will soon find out through our reviews. When there is no resistance in front of a fan, its airflow is at its maximum, but this is not the case for most fans, especially for those used in heatsinks and AIO radiators. Most of the fans that are used in chassis don't face significant resistance.

The maximum static pressure is the fan's wind pressure in a fully enclosed channel. Static pressure is the air pressure the fan can produce in an enclosure. It is measured in Pascals (Pa), inches of water (inH2O), or millimeters of water (mmAq). We will use the latter. The most important thing you need to know is that the fan will not simultaneously output maximum airflow and static pressure values. Airflow and static pressure have a negative correlation. When airflow increases, static pressure decreases, and when static pressure increases, airflow decreases.

Both airflow and static pressure have to do with airflow resistance, called impedance. When parts block the fan's airflow, we have impedance, so to find out the complete P-Q curves of a fan, we have to be somehow able to simulate this impedance. Some users use custom-made

filters or AIO radiators, but these techniques only simulate a single impedance scenario, so they cannot offer complete P-Q curves. The only way to get the entire P-Q curve of a fan is to have variable impedance, which is what an instrument like the LW-9266 does, based on established measuring standards and with full calibration reports.

## Normalized Noise Testing

Testing the fan(s) at full speed only shows a small part of their performance since, in most cases, cooling fans do not operate at full speed. In case they do, their lifetime will be greatly affected besides high noise output. Subsequently, fan speed is typically regulated according to the thermal loads. This is why it is of imperative importance to test and compare each fan under the same conditions. It would be unfair to compare a fan spinning at 3000 RPM with a fan spinning at 1500 RPM. You also have to include the noise output parameter in the comparison, since the fan's rotation speed is not a stable parameter either. E.g., comparing two fans spinning at 1500 RPM is not fair either, since one can output 30 dBA of noise and the other 33 dBA. Noise output has to do with the fan's design too, not only its speed.

Before conducting a complete fan performance evaluation, we have to measure its noise output, since the most important performance of each fan is its performance in normalized noise output. For the normalized noise output tests, we set the fan to speeds with noise output at the following predefined levels: 20/25/30/35/40/45 dBA. We skip the corresponding tests if the fan under the test cannot reach certain noise levels. The speeds shown in the example graph below are measured with the fan in a clear space inside our hemi-anechoic chamber without any obstacles. We set these speed settings on the Long Win machine, but the results can have some minor variance due to external uncontrollable parameters and slight differences in the machine's operations, always within the margin of error.

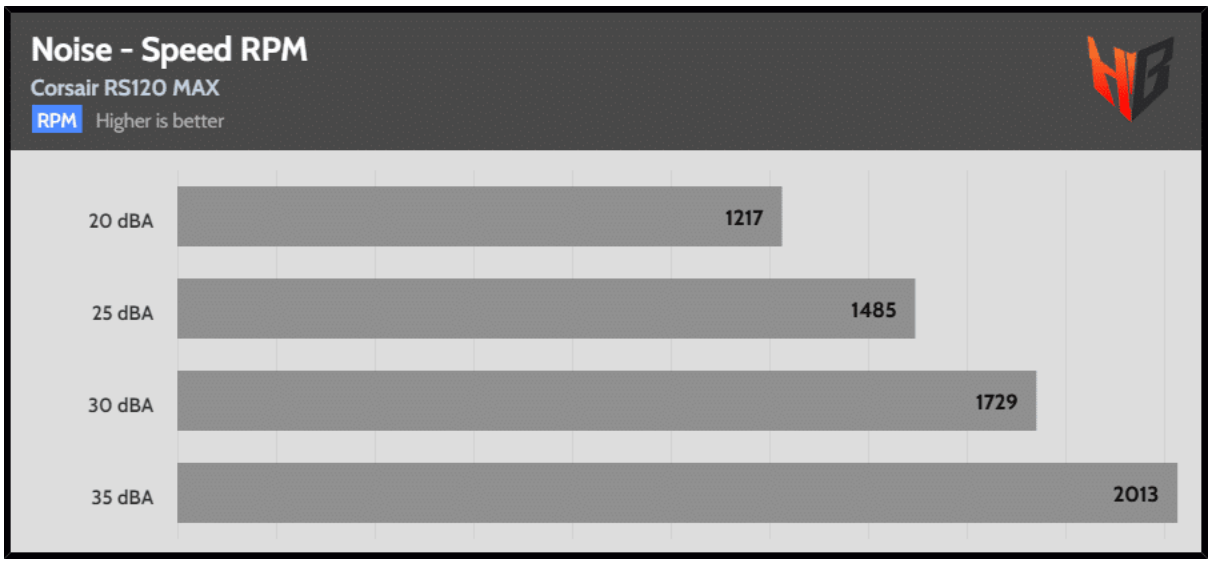


*Picture 1*

## Noise Measurements Procedure

We turn on the sound meter, Bruel & Kjaer G-4 Type 2270 [3], 15 to 30 minutes before starting the measurements to allow it to reach operational temperature. Before we start the measurements, we calibrate the sound meter using the Bruel & Kjaer Sound Calibrator Type 4231 [4].

We install the fan in the chamber in such a position that its airflow goes in the opposite direction to the microphone. We make sure the microphone is installed correctly and in general, we follow all noise testing requirements of the ECMA-74 and ISO 9296 standards [5][6].

We use Corsair's Commander Pro [7] to control the chassis fans, using custom software developed by our team. In addition, the Commander Pro is driven by another passively cooled system that doesn't affect the chamber's noise floor.

Our software allows for precise fan speed adjustments in both RPM and percentage. Hence, we can set a portion of the speed individually for each fan; e.g., setting the fan speed at 50% for a fan with a maximum speed of 1000 RPM will result in a fan speed of 500 RPM (±1%).

We measure the noise the fans produce from their lowest speed up to their maximum speed using 10% intervals. Next, we change the fan speed by reversing the measurements' logic to achieve the corresponding noise output levels for our normalized noise tests, and we record the corresponding fan speeds for later use.

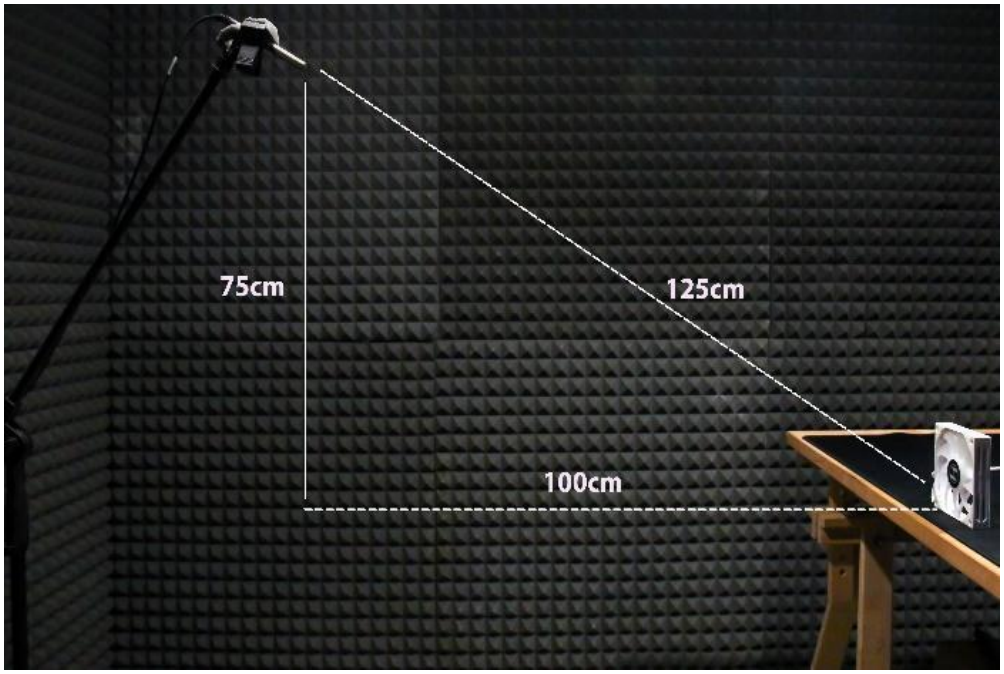


*Picture 2*

## The Phi Fan Performance Standard - PFPS

We named our fan performance Standard, Phi, after the Greek letter «Φ» which among others represents the Golden ratio [8].

The Phi Fan Performance Standard, or PFPS in short, includes both 120mm and 135-140mm fans, but with different requirements for each level. The requirements are set for both airflow and static pressure since these two are the key performance factors for each fan.

All fans that can reach it are rated at 25 dBA normalized noise output, and we take into account these results to rank them in the following categories. Why did we choose this specific noise level for our standard? Because at 25 dBA, a fan can spin fast enough to achieve decent performance, while this noise level isn't high enough to annoy the majority of users. Anything higher or lower than this noise level would be too noisy, or performance would be hugely affected.

What about fans that cannot reach 25 dBA, even at full speed? These fans are designed for very low noise output, so they cannot be compared with other fans at 25 dBA. Rating them at full speed would not be a fair comparison either, since their noise output would then differ from that of the fans they are compared with. For these fans we use the next normalized noise output level of our test routine, 20 dBA. A 120mm or 135/140mm fan whose maximum noise output is below 25 dBA but reaches 20 dBA is rated with the airflow and static pressure measured at 20 dBA normalized noise output, against the 20 dBA requirements listed below. A fan that cannot reach 20 dBA, even at full speed, does not receive a performance level.

In Revision 2.1 (October 2026) we raised the Platinum, Titanium and Diamond requirements for both airflow and static pressure, in both fan categories and at both noise levels, so that Diamond is reserved for the very best fans. Gold now ends where the new Platinum starts; the Silver and Bronze requirements did not change. Every fan already in our database was re-rated with the new requirements from its existing measurements; no fan was measured again.

**PFPS – 120mm Fan Airflow Levels/Requirements – 25 dBA Normalized Noise Output**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥34 CFM & <38 CFM |
| Silver | ≥38 CFM & <42 CFM |
| Gold | ≥42 CFM & <48 CFM |
| Platinum | ≥48 CFM & <53 CFM |
| Titanium | ≥53 CFM & <57 CFM |
| Diamond | ≥57 CFM |

**PFPS – 120mm Fan Static Pressure Levels/Requirements – 25 dBA Normalized Noise Output**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥0.8 mmAq & <1.0 mmAq |
| Silver | ≥1.0 mmAq & <1.25 mmAq |
| Gold | ≥1.25 mmAq & <1.65 mmAq |
| Platinum | ≥1.65 mmAq & <2.1 mmAq |
| Titanium | ≥2.1 mmAq & <2.5 mmAq |
| Diamond | ≥2.5 mmAq |

**PFPS – 135/140mm Fan Airflow Levels/Requirements – 25 dBA Normalized Noise Output**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥45 CFM & <50 CFM |
| Silver | ≥50 CFM & <55 CFM |
| Gold | ≥55 CFM & <62 CFM |
| Platinum | ≥62 CFM & <67 CFM |
| Titanium | ≥67 CFM & <72 CFM |
| Diamond | ≥72 CFM |

**PFPS – 135/140mm Fan Static Pressure Levels/Requirements – 25 dBA Normalized Noise Output**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥0.7 mmAq & <0.9 mmAq |
| Silver | ≥0.9 mmAq & <1.1 mmAq |
| Gold | ≥1.1 mmAq & <1.5 mmAq |
| Platinum | ≥1.5 mmAq & <1.85 mmAq |
| Titanium | ≥1.85 mmAq & <2.3 mmAq |
| Diamond | ≥2.3 mmAq |

The 20 dBA requirements express the same performance levels at the lower noise output; they are not a separate standard. We derived them from our fan database in October 2026. For every fan measured at both 25 dBA and 20 dBA normalized noise output (143 fans of 120mm and 51 fans of 135/140mm), we calculated the ratio of its airflow, and of its static pressure, at 25 dBA to the same value at 20 dBA. Each 25 dBA requirement was then divided by the median of these ratios: 1.221 for the airflow and 1.429 for the static pressure of 120mm fans, and 1.196 and 1.386 respectively for 135/140mm fans. These ratios are fixed for this revision of the standard and are not recalculated as new fans are tested.

Rating the same fans with both sets of requirements, the level obtained at 20 dBA is the same as the level obtained at 25 dBA for 69% to 88% of them, depending on the category, and only 2 of the 388 comparisons differ by more than one level. The rating of a fan at 20 dBA is always based on its own measurement at 20 dBA normalized noise output; the ratios are used only to set the requirements, never to estimate a fan's performance at 25 dBA.

**PFPS – 120mm Fan Airflow Levels/Requirements – 20 dBA Normalized Noise Output (fans that cannot reach 25 dBA)**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥27.8 CFM & <31.1 CFM |
| Silver | ≥31.1 CFM & <34.4 CFM |
| Gold | ≥34.4 CFM & <39.3 CFM |
| Platinum | ≥39.3 CFM & <43.4 CFM |
| Titanium | ≥43.4 CFM & <46.7 CFM |
| Diamond | ≥46.7 CFM |

**PFPS – 120mm Fan Static Pressure Levels/Requirements – 20 dBA Normalized Noise Output (fans that cannot reach 25 dBA)**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥0.56 mmAq & <0.70 mmAq |
| Silver | ≥0.70 mmAq & <0.88 mmAq |
| Gold | ≥0.88 mmAq & <1.15 mmAq |
| Platinum | ≥1.15 mmAq & <1.47 mmAq |
| Titanium | ≥1.47 mmAq & <1.75 mmAq |
| Diamond | ≥1.75 mmAq |

**PFPS – 135/140mm Fan Airflow Levels/Requirements – 20 dBA Normalized Noise Output (fans that cannot reach 25 dBA)**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥37.6 CFM & <41.8 CFM |
| Silver | ≥41.8 CFM & <46.0 CFM |
| Gold | ≥46.0 CFM & <51.8 CFM |
| Platinum | ≥51.8 CFM & <56.0 CFM |
| Titanium | ≥56.0 CFM & <60.2 CFM |
| Diamond | ≥60.2 CFM |

**PFPS – 135/140mm Fan Static Pressure Levels/Requirements – 20 dBA Normalized Noise Output (fans that cannot reach 25 dBA)**

| Performance Levels | Requirements |
|---|---|
| Bronze | ≥0.51 mmAq & <0.65 mmAq |
| Silver | ≥0.65 mmAq & <0.79 mmAq |
| Gold | ≥0.79 mmAq & <1.08 mmAq |
| Platinum | ≥1.08 mmAq & <1.33 mmAq |
| Titanium | ≥1.33 mmAq & <1.66 mmAq |
| Diamond | ≥1.66 mmAq |

## Performance Badges & Ratings

Since we don't want to confuse users, we used the highly familiar metal and carbon ratings that we already use for our PSU efficiency ratings: Bronze, Silver, Gold, Platinum, Titanium, and Diamond.

There are two fan categories, the most popular ones: 120mm and 135/140mm. Larger fans, such as 148mm and 150mm models, are rated with the 135/140mm requirements at 25 dBA normalized noise output; the 20 dBA route is not available to them, so a larger fan that cannot reach 25 dBA does not receive a performance level. There are also two badges for the fan's main performance factors: airflow and static pressure.

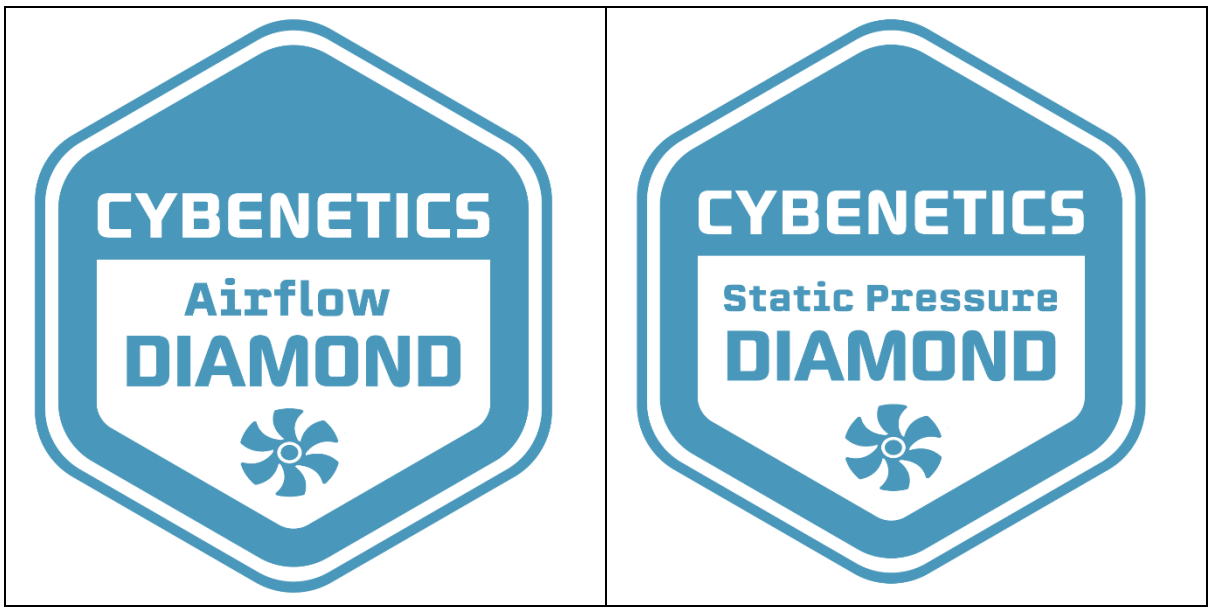


When a fan is rated at 20 dBA normalized noise output, the evaluation report and the certificate state this noise level next to the rating.

## Measurement Uncertainty

Measurement uncertainty is the quantified doubt about a measurement result. It shows the range within which the true value is expected to lie. Uncertainty for the fan aerodynamic measurements was evaluated in accordance with JCGM 100:2008 (GUM) and ISO/IEC 17025:2017.

The reported expanded uncertainty U is the combined standard uncertainty multiplied by a coverage factor k = 2, corresponding to a confidence level of approximately 95 %.

The Air Flow Measurement's Uncertainty is RELATIVE to the reading at 1.23176 %: $U(Q) = 2 \cdot \sqrt{[(1.8200\ \text{CFM})^2 + (0.0123176 \cdot Q)^2]}$, k = 2, valid over the declared measuring range 2.4 – 250 CFM. That gives ±3.69 CFM at 25 CFM, ±3.84 at 50, ±4.29 at the 92.1 CFM control point, ±5.19 at 150 and ±7.15 CFM at 250 CFM. Air-flow scatter tracks the reading rather than staying fixed, so a single absolute figure understates the uncertainty at high flow.

The Static Pressure Measurement's Uncertainty is ±0.6727 Pa, valid over the standard measuring range 0 – 20 mmAq (0 – 196.1 Pa). The apparatus can be extended to 100 mmAq (981 Pa) using the high static pressure throttle device; this extended range is used only rarely and its uncertainty has not yet been separately verified — see the verification action in the controlled record P19-F01 rev.07, 07-09-2026.

Uncertainty is stated across the declared measuring ranges rather than at a single operating point, because the deliverable of this standard is a complete P–Q characteristic which traverses the whole range in every test.

Air Flow Measurement Uncertainty Budget

| Source of Uncertainty | Standard Uncertainty, u(xi) (CFM) |
|---|---|
| LW-9266 instrument accuracy (Type B) | 1.750 |
| Repeatability, control sample (Type A) | 1.135 |
| Calibration (Type B) | 0.500 |
| Combined Standard Uncertainty (RSS): | 2.145 |
| Expanded Uncertainty U (k=2, norm): | 4.290 |

Static Pressure Measurement Uncertainty Budget

| Source of Uncertainty | Standard Uncertainty, u(xi) (Pa) |
|---|---|
| Repeatability, control sample (Type A) | 0.328 |
| LW-9266 calibration (Type B) | 0.075 |
| Combined Standard Uncertainty (RSS): | 0.336 |
| Expanded Uncertainty U (k=2, norm): | 0.673 |

Repeatability is evaluated as Type A from repeated laboratory measurements on a control sample and is treated as an absolute quantity across the declared range. The LW-9266 manufacturer specification is applied separately as the Type B instrument-accuracy contribution.

## Decision Rule

Badges are awarded by simple acceptance. A fan's measured air flow and static pressure at 25 dBA normalized noise output (or at 20 dBA, for fans that cannot reach 25 dBA) are compared directly with the corresponding level requirements listed above; the measurement uncertainty is not added to or subtracted from the measured value before that comparison. This is a shared-risk rule of the kind permitted by ISO/IEC 17025:2017 clause 7.8.6.2, and it means that where a result falls close to a level boundary the true value may lie on either side of it.

Where a measured value lies within one expanded uncertainty of a level boundary, we repeat the evaluation on three independent runs, each with its own noise measurement, and compare the mean of the three against the boundary. If the mean still falls within that margin, the lower level is awarded.

## Epilogue

This article was a brief introduction to the world of fan testing and a first look at our testing methodology. Providing an objective representation of a fan’s performance is a delicate task, requiring experience in both sound measurement and aerodynamics. The equipment used for our testing is the industry standard, of the highest quality, and properly maintained and operated. Moreover, we have tested numerous fans so far, in the process of refining our methods. Subsequently, the information and testing results we provide are both accurate and indicative of real-world performance.

# References

[1] LW-9266 Fan PQ Performance Measurement Apparatus.
http://www.longwin.com/english/product/9266.html (last accessed on 3 October 2026)
[2] Picoscope TC-08. https://www.picotech.com/data-logger/picolog-tc-08-thermocouple-data-logger
(last accessed on 3 October 2026)
[3] https://www.hbkworld.com/en/products/instruments/handheld/hand-held-software/sound-level-meter-apps-2250-2270/pre-packaged-software-2270-bz-7222 (last accessed on 3 October 2026)
[4] https://www.hbkworld.com/en/products/transducers/acoustic/acoustic-calibrators/microphone/4231
(last accessed on 3 October 2026)
[5] Standard ECMA-74 Measurement of Airborne Noise Emitted by Information Technology and Telecommunications Equipment
https://ecma-international.org/publications-and-standards/standards/ecma-74/
(last accessed on 3 October 2026)
[6] ISO 9296:2017 Acoustics - Declared noise emission values of information technology and telecommunications equipment https://www.iso.org/standard/32303.html
(last accessed on 3 October 2026)
[7] https://www.corsair.com/eu/en/p/accessories/cl-9011110-ww/icue-commander-pro-smart-rgb-lighting-and-fan-speed-controller-cl-9011110-ww (last accessed on 3 October 2026)
[8] Golden ratio https://en.wikipedia.org/wiki/Golden_ratio (last accessed on 3 October 2026)
[9] ANSI/AMCA Standard 210-25 / ANSI/ASHRAE Standard 51-25, Laboratory Methods of Testing Fans for Certified Aerodynamic Performance Rating. Air Movement and Control Association International / ASHRAE. (Supersedes ANSI/AMCA 210-16 / ASHRAE 51-16.)
[10] ISO 5801, Fans – Performance testing using standardized airways.
[11] ISO/IEC 17025:2017, General requirements for the competence of testing and calibration laboratories.
[12] JCGM 100:2008 (GUM), Evaluation of measurement data – Guide to the expression of uncertainty in measurement. Joint Committee for Guides in Metrology.
[13] ECMA-74, 22nd edition, December 2025, Measurement of Airborne Noise emitted by Information Technology and Telecommunications Equipment. ECMA International, Geneva.
[14] ISO 7779:2018, Acoustics – Measurement of airborne noise emitted by information technology and telecommunications equipment.